PHILIPS MEDICAL SYSTEMS

NEWSLETTER **SERVICE**

ISSUED BY	: PMS DMC HAMBURG	REFERENCE NO.	: XRD HAMBURG 134
PUBLICATION NO.	: 4512 980 64251 REV AA	DATE	: FEBRUAR 2008

INFORMATION FOR : FSE SPECIALIST

AGENT 5.1 FAILURE IN DOSE RATE CONTROL PROGRAMMING

Problems occur during the programming of "Dose Rate Control" data sets Optimus RAD / RF / C with AgenT version 5.1

The CHAMBER.TDL data set takes wrong parameters depending on the chamber type selected.

As a work-around two solutions are available:

1. **Before the new AGent 5.1 version is installed**
   Save the original chamber.tdl data file in a new directory.
   Install the new AGenT version and replace the existing file chamber.tdl of 23.11.2007 with the old saved file.

2. **After the new new AGenT version 5.1 has been installed**
   Download the chamber.tdl data file from the Optimus firmware download area of the InCenter and replace the existing file of 23.11.2007.

THIS DOCUMENT AND THE INFORMATION CONTAINED IN IT IS PROPRIETARY AND CONFIDENTIAL INFORMATION OF PHILIPS MEDICAL SYSTEMS ("PHILIPS") AND MAY NOT BE REPRODUCED, COPIED IN WHOLE OR IN PART, ADAPTED, MODIFIED, DISCLOSED TO OTHERS, OR DISSEMINATED WITHOUT THE PRIOR WRITTEN PERMISSION OF THE PHILIPS LEGAL DEPARTMENT.
(C) 2008 KONINKLIJKE PHILIPS ELECTRONICS N.V.
ALL RIGHTS RESERVED

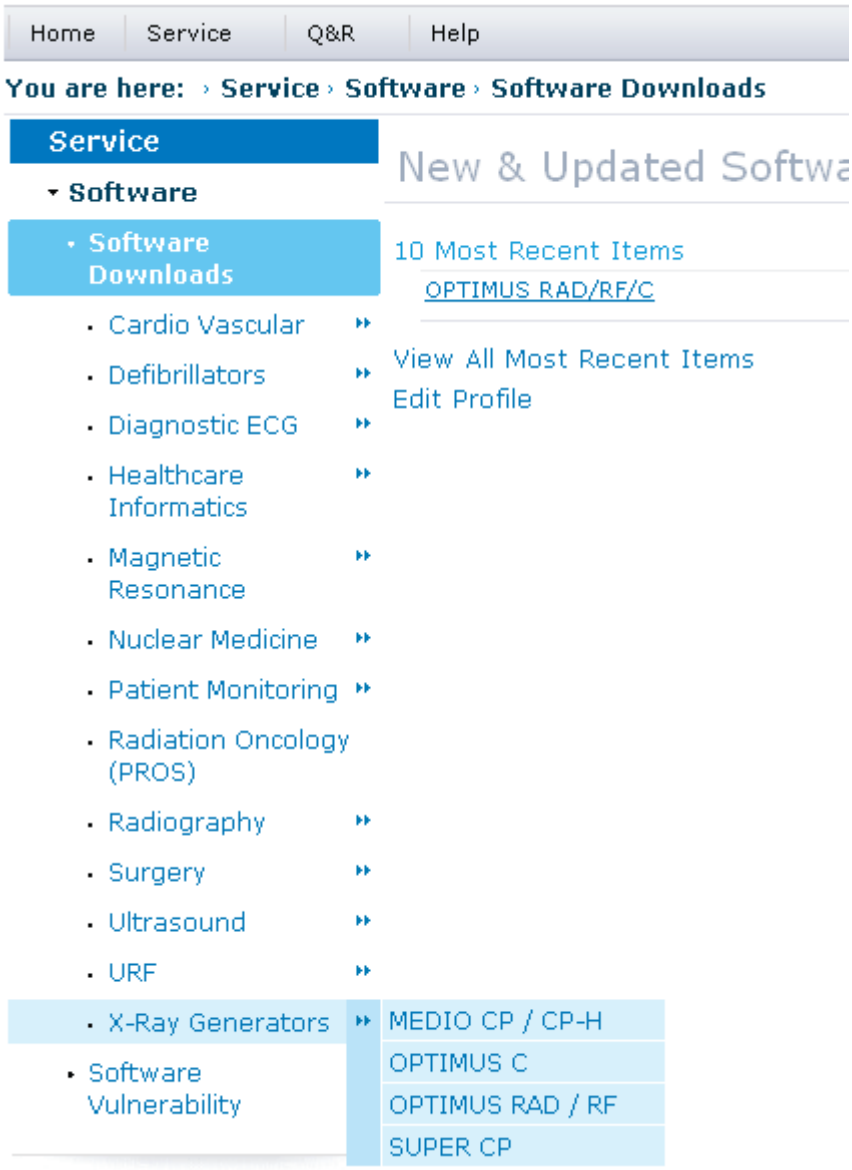

THIS DOCUMENT AND THE INFORMATION CONTAINED IN IT IS PROPRIETARY AND CONFIDENTIAL INFORMATION OF PHILIPS MEDICAL SYSTEMS ("PHILIPS") AND MAY NOT BE REPRODUCED, COPIED IN WHOLE OR IN PART, ADAPTED, MODIFIED, DISCLOSED TO OTHERS, OR DISSEMINATED WITHOUT THE PRIOR WRITTEN PERMISSION OF THE PHILIPS LEGAL DEPARTMENT.
(C) 2008 KONINKLIJKE PHILIPS ELECTRONICS N.V.
ALL RIGHTS RESERVED

PHILIPS CUSTOMerCARE InCenter

back to InCenter

Download OPTIMUS RAD/RF/C

modified: 28.01.2008

	Description (click for further info)	FCO	File (click to download)	Size	Issued
	Tube data file, vers. 20.02.04		tube_r3.zip	151k	15.04.2005
	Troubleshooting and experience data collection		CD_field_engineer.zip	92.893k	19.04.2006
	Agent = XRGSCOPE successor communication software				
	Service Software - Installation script and service tool for Optimus RAD/RF/C X-ray generators (AGenT)		AGenT_43.zip	11.766k	15.12.2005
	Firmware Optimus RAD-RF Release 3.7 to be loaded to the Agent 4.3 directory		omcur3l7.tdl	2.140k	06.06.2007
	Problems during programming of "Dose Rate Control" data sets Optimus RAD / RF / C with AgenT version 5.1 The CHAMBER.TDL data set takes wrong parameters depending on the chamber type selected. As a work around download the chamber.tdl data file from the Optimus firmware download area of the InCenter and replace the existing file of 23.11.2007.		chamber.tdl	12k	28.01.2008

ROPRIETARY NOTICE CSIP LEVEL 1:

THIS DOCUMENT AND THE INFORMATION CONTAINED IN IT IS STRICTLY RESERVED FOR CURRENT PHILIPS MEDICAL SYSTEMS ("PHILIPS") PERSONNEL, PHILIPS LICENSED REPRESENTATIVES AND PHILIPS CUSTOMERS WHO HAVE PURCHASED A VALID SERVICE AGREEMENT FOR USE BY THE CUSTOMER'S DESIGNATED IN-HOUSE SERVICE EMPLOYEE ON EQUIPMENT LOCATED AT THE CUSTOMER'S DESIGNATED SITE. USE OF THIS DOCUMENT BY UNAUTHORIZED PERSONS IS STRICTLY PROHIBITED. THIS DOCUMENT MUST BE RETURNED TO PHILIPS WHEN THE USER IS NO LONGER LICENSED AND IN ANY EVENT UPON PHILIPS' FIRST WRITTEN REQUEST.

LIABILITY / WARRANTY DISCLAIMER:

PHILIPS PROVIDES THIS DOCUMENT WITHOUT WARRANTY OF ANY KIND, IMPLIED OR EXPRESSED, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. PHILIPS HAS TAKEN CARE TO ENSURE THE ACCURACY OF THIS DOCUMENT. HOWEVER, PHILIPS ASSUMES NO LIABILITY FOR ERRORS OR OMISSIONS AND RESERVES THE RIGHT TO MAKE CHANGES WITHOUT FURTHER NOTICE TO ANY PRODUCTS HEREIN TO IMPROVE RELIABILITY, FUNCTION, OR DESIGN. PHILIPS MAY MAKE IMPROVEMENTS OR CHANGES IN THE PRODUCT(S) OR PROGRAM(S) DESCRIBED IN THIS DOCUMENT AT ANY TIME.

THIS DOCUMENT AND THE INFORMATION CONTAINED IN IT IS PROPRIETARY AND CONFIDENTIAL INFORMATION OF PHILIPS MEDICAL SYSTEMS ("PHILIPS") AND MAY NOT BE REPRODUCED, COPIED IN WHOLE OR IN PART, ADAPTED, MODIFIED, DISCLOSED TO OTHERS, OR DISSEMINATED WITHOUT THE PRIOR WRITTEN PERMISSION OF THE PHILIPS LEGAL DEPARTMENT.

(C) 2008 KONINKLIJKE PHILIPS ELECTRONICS N.V.

ALL RIGHTS RESERVED